

• ABOUT US •

Driven by the passion for innovation, we at Dr Trust endeavour to provide our customers with the latest medical inventions with an objective to promote good health and wellness all around the world. All the medical devices and health monitors provided by Dr Trust are supported by accurate, latest and ground breaking technologies, innovated at our headquarter in NY, USA. All our products adhere to the most stringent CE and FDA guidelines and are strongly recommended by doctors and health practitioners. Our products are designed in the utmost exemplary ways to ensure that their accuracy and convenience are unrivalled. The ease of their use and operation makes them even more suitable for users of all age groups.

Dr Trust strives to enhance the quality of lifestyle by providing with the most trusted and innovative health care and wellness products. Being a renowned global leader in health care products, Dr Trust ensures that our technically efficient team works dynamically and tirelessly to provide the best of the medical devices to our clients. The products that we have to offer are suitably designed for use at homes, laboratories and hospitals.

Our ground breaking solutions allow you to monitor your health in the easiest ways possible. In today's era when all of our lives are too hassled to handle, it becomes a bit difficult to pay attention to our health. But it has now become easier with the coming of the monitoring devices which can be conveniently used at homes and even on the go.

We bring to you a variety of best self medical devices, trusted and used by Doctors, medical professionals and home users all over the world.

Dr Trust BP Check Pro-123

• QUICK STARTUP GUIDE •

Step 1

Insert the batteries and press the TIME button to check the date on the display.

Step 2

Press User button to select the user (User 1, User 2).

Step 3

Set time and date by pressing Time and Memory button.

Step 4

Sit comfortably in a chair with uncrossed legs next to table and roll up you are left arm sleeve.

Step 5

Position the cuff appropriately and set preferred measuring mode (Standard Mode and AFIB Mode) to start measurement.

Step 6

Press the ON/OFF button, the display will show result within few seconds.



123

● TABLE OF CONTENTS ●

1. INTRODUCTION	4
1.1. Features of the Dr Trust BP Check Pro-123	
1.2. Important information about self-measurement	
2. IMPORTANT INFORMATION ON THE SUBJECT OF BLOOD-PRESSURE AND ITS MEASUREMENT	5
2.1. How does high/low blood-pressure arise?	
2.2. Which values are normal?	
3. IMPORTANT FACTS ABOUT ATRIAL FIBRILLATION (AFIB)	8
4. THE VARIOUS COMPONENTS OF THE BLOOD-PRESSURE MONITOR	9
5. PUTTING THE BLOOD-PRESSURE MONITOR INTO OPERATION	10
5.1. Inserting the batteries	
5.2. Reading the set date	
5.3. User selection and setting the time / date	
6. CARRYING OUT A MEASUREMENT	12
6.1. Before the measurement	
6.2. Common sources of error	
6.3. Fitting the cuff	
6.4. Measuring procedure	
6.5. Discontinuing a measurement	
6.6. Memory – storage and recall of the measurements	
6.7. Memory – cancellation of all measurements	

7. APPEARANCE OF THE HEART ARRHYTHMIA INDICATOR FOR EARLY DETECTION	19
8. APPEARANCE OF THE ATRIAL FIBRILLATION INDICATOR FOR EARLY DETECTION	20
9. ERROR MESSAGES / MALFUNCTIONS	20
10. CARE AND MAINTENANCE, RECALIBRATION	23
11. BATTERY LIFE	23
12. SAFETY, CARE AND DISPOSAL	23
13. REFERENCE TO STANDARDS	25
14. REMARK	25
15. TECHNICAL SPECIFICATIONS	26
16. MANUFACTURER'S DECLARATION	28
17. Contact Us	35
18. About Us	36



● 1. INTRODUCTION ●

The blood-pressure monitor Dr Trust BP Check Pro-123 (with integrated time/date display) is a fully automatic, digital blood-pressure measuring device for use on the arm, which enables very fast and reliable measurement of the systolic and diastolic blood-pressure as well as the pulse frequency by way of the oscillometric method of measurement.

The device offers very high and clinical tested measurement accuracy and has been designed to provide maximum of user-friendliness.

Before using, please read this instruction manual carefully and keep it in a safe place. For further questions about blood-pressure and its measurement, please contact your doctor.

⚠ Attention

1.2. Important information about self-measurement

- Substitution of a different component might result in measurement error.
- cuff is replaceable only by an original one.
- Do not use with neonatal patients.
- It will cause harmful injury to the patient or effect the blood pressure due to connection tubing kinking.
- Too frequent measurements can cause injury to the patient due to blood flow interference.
- The application of the cuff over a wound can cause further injury.
- The application of the cuff and its pressurization on any limb where intravascular access or therapy, or an arteriovenous (A-V) shunt, is present because of temporary interference to blood flow and could result in injury to the patient.
- Do not let the cuff and its pressurization on the arm on the side of a mastectomy

- The need to check that operation of the automated sphygmomanometer does not result in prolonged impairment of patient blood circulation.
- Not intended to be used together with HF surgical equipment.
- **Do not forget:** self-measurement means control, not diagnosis or treatment. Unusual values must always be discussed with your doctor. Under no circumstances should you alter the dosages of any drugs prescribed by your doctor.
- The pulse display is not suitable for checking the frequency of heart pacemakers!
- In cases of cardiac irregularity (Arrhythmia), measurements made with this instrument should only be evaluated after consultation with the doctor.

Electromagnetic interference

The device contains sensitive electronic components (Microcomputer). Therefore, avoid strong electrical or electromagnetic fields in the direct vicinity of the device (e.g. mobile telephones, microwave cookers). These can lead to temporary impairment of the measuring accuracy.

● 2. IMPORTANT INFORMATION ON THE SUBJECT OF BLOOD-PRESSURE AND ITS MEASUREMENT ●

2.1. How does high/low blood-pressure arise?

The level of blood-pressure is determined in a part of the brain, the so-called circulatory center, and adapted to the respective situation by way of feedback via the nervous system. To adjust the blood-pressure, the strength and frequency of the heart (Pulse), as well as the width of circulatory blood vessels is altered.



The latter is affected by way of fine muscles in the blood-vessel walls. The level of arterial blood-pressure changes periodically during the heart activity: During the «blood ejection» (Systole) the value is maximal (systolic blood-pressure value), at the end of the heart's «rest period» (Diastole) minimal (diastolic blood-pressure value). The blood-pressure values must lie within certain normal ranges in order to prevent particular diseases.

2.2. Which values are normal?

Blood pressure is too high if at rest, the diastolic pressure is above 90 mmHg and/or the systolic blood-pressure is over 160 mmHg. In this case, please consult your doctor immediately. Long-term values at this level endanger your health due to the associated advancing damage to the blood vessels in your body.

Should the systolic blood-pressure values lie between 140 mmHg and 160 mmHg and/or the diastolic blood-pressure values lie between 90 mmHg and 100 mmHg, likewise, please consult your doctor. Furthermore, regular self-checks will be necessary.

With blood-pressure values that are too low, i.e. systolic values under 100 mmHg and/or diastolic values under 60 mmHg, likewise, please consult your doctor. Even with normal blood-pressure values, a regular self-check with your blood-pressure monitor is recommended. In this way you can detect possible changes in your values early and react appropriately. If you are undergoing medical treatment to control your blood pressure, please keep a record of the level of your blood pressure by carrying out regular self-measurements at specific times of the day. Show these values to your doctor. **Never use the results of your measurements to alter independently the drug doses prescribed by your doctor.**

Table for classifying blood-pressure values (unit: mmHg) according to World Health Organization:

Range	Systolic Blood pressure	Diastolic Blood-pressure	Measures
optimum	between 100 and 120	between 60 and 80	Self-check
normal	between 120 and 129	between 80 and 84	Self-check
high to normal	between 130 and 139	between 85 and 89	Consult your doctor
slight hypertension	between 140 and 159	Between 90 and 99	Seek medical advice
medium hypertension	between 160 and 179	Between 100 and 109	Seek medical advice
strong hypertension	Higher than 180	Higher than 110	Urgently seek medical advice!

Further information

- If your values are mostly standard under resting conditions but exceptionally high under conditions of physical or psychological stress, it is possible that you are suffering from so-called «labile hypertension». Please consult your doctor if you suspect that this might be the case.
- Correctly measured diastolic blood-pressure values above 120 mmHg require immediate medical treatment.



3. IMPORTANT FACTS ABOUT ATRIAL FIBRILLATION (AFIB)


What is Atrial Fibrillation (AFIB)?

Normally, your heart contracts and relaxes to a regular beat. Certain cells in your heart produce electrical signals that cause the heart to contract and pump blood. Atrial fibrillation occurs when rapid, disorganized electrical signals are present in the heart's two upper chambers, called the atria; causing them to contract irregularly (this is called fibrillation). Atrial fibrillation is the most common form of heart arrhythmia or irregular heartbeat. It often causes no symptoms, yet it significantly increases your risk of stroke. You will need a doctor to help you control the problem.

How does AFIB impact my family or me?



People with AFIB have a five-fold higher risk of getting stroke. Since the chance of having a stroke increases with age, AFIB screening is recommended for people over 65 years and older. However, for people from the age of 50 years with high blood pressure (hypertension), diabetes, coronary heart failure or have had a previous stroke AFIB screening is also recommended. Early ADVANCE AFIB followed by adequate treatment can significantly reduce the risk of getting stroke. In young people AFIB screening is not recommended as it could generate false positive results and unnecessary anxiety. In addition, young individuals with AFIB have a relatively low risk of getting stroke as compared to elder people. ADVANCE AFIB detection provides a convenient way to screen for AFIB. Knowing your blood pressure and knowing whether you or your family members have AFIB can help reduce the risk of stroke. ADVANCE AFIB detection provides a convenient way to screen for AFIB whilst taking your blood pressure.

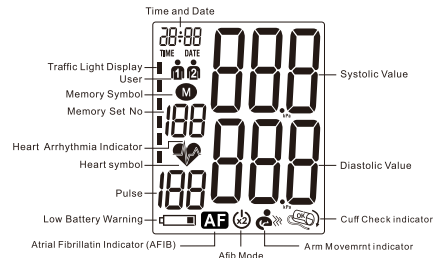
4. THE VARIOUS COMPONENTS OF THE BLOOD-PRESSURE MONITOR



5. PUTTING THE BLOOD-PRESSURE MONITOR INTO OPERATION

5.1. Inserting the batteries

- a) Insert the batteries (4 x size AAA1.5V), thereby observing the indicated polarity.
- b) If the battery warning  icon appears in the display, the batteries remain 20% power to warn user the batteries will be run out.
- c) If the battery warning  icon appears in the display, the batteries are empty and must be replaced by new ones

Attention! After the battery warning  icon appears, the device is blocked until the batteries have been replaced.

- Please use «AAA» Long-Life or Alkaline 1.5V batteries. The use of 1.2V Accumulators is not recommended.
- If the blood-pressure monitor is left unused for long periods, please remove the batteries from the device.

5.2. Reading the set date

Please press the TIME button and the date will be shown in the display.

5.3. User selection and setting the time / date

User selection: This advanced blood pressure monitor allows you to track blood pressure readings for 2 individuals independently

- a) Before measurement, make sure you set the unit for the intended user. The unit can track results for 2 individuals. (User 1, User 2)
- b) Press the user button. The display now indicates the set user, during which the set user blink, to confirm, press ON/OFF button
- c) We suggest the first person to take their pressure to be User 1.

Setting the time, date

This blood-pressure monitor incorporates an integrated clock with date display. This has the advantage, that at each measurement procedure, not only the blood-pressure values are stored, but also the exact moment of the measurement. After new batteries have been inserted, the clock begins to run TIME 12:00 and DATE 1-01. You must then re-enter the date and current time. For this, please proceed as follows.

1. Press the TIME button for at least 3 seconds firstly, user icon will blink. Then press TIME button again the display now indicates the set year, during which the four characters blink.
2. The correct year can be entered by pressing the MEMORY button
3. Press the TIME button again. The display now switches to the current date, during which the first character (month) blinks.
4. The corresponding month can now be entered by pressing the MEMORY button.
5. Press the TIME button again. The last two characters (day) are now blinking
6. The corresponding day can now be entered by pressing the MEMORY button.
7. Press the TIME button again. The display now switches to the current time, during which the first character (Hour) blinks
8. The corresponding hour can now be entered by pressing the MEMORY button.
9. Press the TIME button again. The last two characters (Minutes) now blink.
10. The exact time can now be entered by pressing the MEMORY button
11. Press TIME button: the unit of measurement will flash.
12. Press the "MEMORY to set the unit of measurement (mmHg or kPa)
13. Once you have made your settings, press the TIME button (or TIME / DATE or TIME). The setting is confirmed and the clock starts running.



14. Now after all settings have been made, press the TIME button once again. The date is briefly displayed and then the time. The input is now confirmed and the clock begins to run.

Further Information

With each press of the button (TIME, MEMORY) one input is made (e.g. switching over from hours to minutes mode, or altering the value by +1). However, if you keep the respective button depressed, you can switch more quickly to find the desired value respectively.

6. CARRYING OUT A MEASUREMENT

6.1. Before the measurement

- Avoid eating, smoking as well as all forms of exertion directly before the measurement. All these factors influence the measurement result. Try and find time to relax by sitting in an armchair in a quite atmosphere for about ten minutes before the measurement.
- Measure always on the same arm (normally left).
- Attempt to carry out the measurements regularly at the same time of day, since the blood-pressure changes during the course of the day.

6.2. Common sources of error

- Note: Comparable blood-pressure measurements always require the same conditions! These are normally always quiet conditions.


- All efforts by the patient to support the arm can increase the blood-pressure. Make sure you are in a comfortable, relaxed position and do not activate any of the muscles in the measurement arm during the measurement. Use a cushion for support if necessary.
- The performance of the automated sphygmomanometer can be affected by extremes of temperature, humidity and altitude.
- Avoid compression or restriction of the connection tubing.
- A loose cuff causes false measurement values.
- With repeated measurements, blood accumulates in the respective arm, which can lead to false results. Correctly executed blood-pressure measurements should therefore first be repeated after a 5 minutes pause or after the arm has been held up in order to allow the accumulated blood to flow away (after at least 3 minutes).

6.3. Fitting the cuff

Insert air connector into air outlet shown in left photo and please make sure the fitting of the air connector completely and properly to avoid air leakage.




- a) The distance between the edge of cuff and the elbow should be approx. 2-3cm

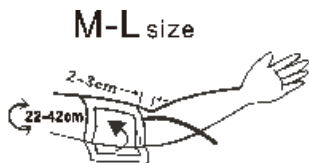

- b) Secure the cuff with the Velcro fastener, so that it lies comfortably and not too tight, whereby 2 finger space should remain between the cuff and the arm.

- c) Lay the arm on a table, with the palm upwards. Support the arm a little with a rest (cushion), so that the cuff rests at about the same height as the heart. Take care, that the cuff lies free. Remain so for 2 minutes sitting quietly, before beginning with the measurement.






- d) Let legs uncrossed, feet flat on the floor, back and arm supported.

6.4. Measuring procedure

6.4.1 Measuring in standard mode

In this mode has arrhythmia detection but no Afib detection. After the cuff has been appropriately positioned, the measurement can begin:

- a) Press the ON/OFF button: the pump begins to inflate the cuff. In the display, the increasing cuff-pressure is continually displayed.
- b) **Cuff fitting detection:** the icon  will appear and blink during measuring if cuff was fit too loose. The icon  will appear during measuring if cuff was fit well.
- c) **Arm movement detection during measuring:** the icon  will appear, if a movement was detected which may influence accuracy, due to the movement not too serious, the measuring can be continuous (if the movement is too serious, Err2 displayed).
- d) After reaching the inflation pressure, the pump stops, and the pressure slowly falls away. The cuff-pressure is displayed during the measurement. When the device has detected the pulse, the heart symbol in the display begins to blink and for every pulse beat.



The measured systolic and diastolic blood-pressure values as well as the pulse frequency are now displayed.


Example (Fig.): Systole 126, Diastole 85, Pulse 78



The measurement results are displayed, until you switch the device off. If no button is pressed for 3 minutes, the device switches automatically off, to save the batteries.


6.4.2 Measuring in Afib Mode (2-measurement mode)

In Afib mode, 2 measurements are automatically taken in succession and the result is then automatically analyzed and displayed. Because blood pressure constantly fluctuates, a result determined in this way is more reliable than one produced by a single measurement.

- After pressing the ON/Afib button more than one seconds, the  symbol appears in the display.

- The middle, left hand section of the display shows a 1, 2 to indicate which of the 2 measurements is currently being taken.

- There is a break of 15 seconds between the measurements
A countdown indicates the remaining time.



- The individual results are not displayed. Your blood pressure will only be displayed after all 2 measurements are taken.

- Do not remove the cuff between measurements.

- If one of the individual measurements was questionable, a third one is automatically taken.

In the measuring:

After reaching the inflation pressure, the pump stops, and the pressure slowly falls away. The cuff-pressure is displayed during the measurement. When the device has detected the pulse, the heart symbol in the display begins to blink





Measured result:

The measured systolic and diastolic blood-pressure values as well as the pulse are now displayed.

Example 1:


Systole 128, Diastole 86, Pulse 68, Afib detected.

Icon of Arrhythmia  and Afib  will be appeared
Arm movement detected and cuff fit too loose detected



Example 1

Example 2:

Systole 128, Diastole 86, Pulse 68, arrhythmia  detected, but no Afib detected.

Arm movement detected and cuff fit well



Example 2

The measurement results are displayed until you switch the device off. If no button is pressed for 3 minutes, the device switches automatically off




6.5. Discontinuing a measurement

If it is necessary to interrupt a blood pressure measurement for any reason (e.g., the patient feels unwell), the "ON/OFF" power button can be pressed at any time. The device then immediately lowers the cuff-pressure automatically.

6.6. Memory – storage and recall of the measurements


The blood-pressure monitor automatically stores each of the last 120 measurement values. By pressing the MEMORY button, an average value of the last 3 measurements as well as the last measurement and the further last 120 measurements (MR119, MR118, ..., MR1) can be displayed one after the other

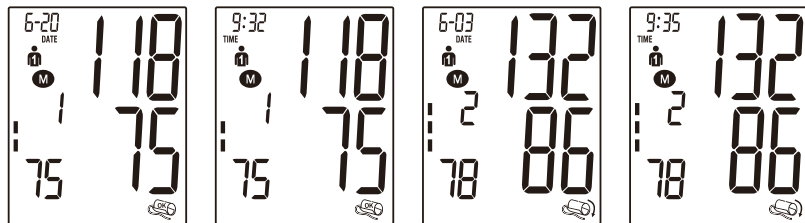


(MR1: Values of the last measurement) (MR2-MR120: Values of the measurement before MR1)

6.7. Memory – cancellation of all measurements Attention!

Before you delete all readings stored in the memory, make sure you will not need refer to the readings at a later date. Keeping a written record is prudent and may provide additional information for your doctor's visit. In order to delete all stored readings, depress the MEMORY button for at least 5 seconds, the display will show the symbol «CL» and then release the button. To permanently clear the memory, Press the MEMORY button while «CL» is flashing.



7. APPEARANCE OF THE HEART ARRHYTHMIA INDICATOR FOR EARLY DETECTION

The Symbol  indicates that certain pulse irregularities were detected during the measurement. In this case, the result may deviate from your normal blood pressure – repeat the measurement. In most cases, this is no cause for concern. However, if the symbol appears on a regular basis (e.g. several times a week with measurements taken daily) we advise you to tell your doctor. Please show your doctor the following explanation Information for the doctor on frequent appearance of the Arrhythmia indicator This instrument is an oscillometric blood pressure monitor that also analyses pulse frequency during measurement. The instrument is clinically tested. The arrhythmia symbol is displayed after the measurement, if pulse irregularities occur during measurement. If the symbol appears more frequently (e.g., several times per week on measurements performed daily) we recommend the patient to seek medical advice. The instrument does not replace a cardiac examination but serves to detect pulse irregularities at an early stage.



● 8. APPEARANCE OF THE ATRIAL FIBRILLATION INDICATOR FOR EARLY DETECTION ●

This device can detect Atrial Fibrillation (AFIB). This icon **AF** indicates that atrial fibrillation was detected during the measurement. If the AFIB symbol appears after having performed a full blood pressure measurement episode (triplicate measurements), you are advised to wait for one hour and perform another measurement episode (triplicate measurements). If the AFIB symbol appears again, then you are advised to visit your doctor. If after repeated measurement the AFIB symbol is no longer displayed there is no cause for concern. In such case it is recommended to measure again the next day. Keep the arm still during measuring to avoid false readings. This device may not detect atrial fibrillation in people with pacemakers or defibrillators.

● 9. ERROR MESSAGES /MALFUNCTIONS ●

If an error occurs during a measurement, the measurement is discontinued and a corresponding error code is displayed.

Error No.	Possible cause(s)
ERR 1	No pulse has been detected.
ERR 2	Unnatural pressure impulses influence the measurement result. Reason: The arm was moved during the Measurement (Artifact).
ERR 3	The inflation of the cuff takes too long. The cuff is not correctly seated.

ERR 5	The measured readings indicated an unacceptable difference between systolic and diastolic pressures. Take other reading following directions carefully. Contact you doctor if you continue to get unusual readings.
ERR 8	Pressure in cuff is over 290mmHg

Further Information - The level of blood-pressure is subject to fluctuations even with healthy people. Important thereby is, that comparable measurements always require the same conditions (Quiet conditions)! If, in spite of observing all these factors, the fluctuations are larger than 15mmHg, and/or you hear irregular pulse tones on several occasions, please consult your doctor. For licensing, the device has been subjected to strict clinical tests, by which the computer program used to measure the blood-pressure values was tested by experienced specialist doctors in Germany. The same computer program is used in every individual device and has thus also been clinically tested. The manufacture of the devices takes place according to the terms of the European standard for blood-pressure measuring devices (see technical data) You must consult your specialist dealer or chemist if there are technical problems with the blood-pressure instrument. Never attempt to repair the instrument yourself!

Other possible malfunctions and their elimination

If problems occur when using the device, the following points should be checked and if necessary, the corresponding measures are to be taken:



Malfunction	Remedy
The display remains empty when the instrument is switched on although the batteries are in place.	1. Check batteries for correct polarity and if necessary insert correctly. 2. If the display is unusual, re-insert batteries or exchange them.
The device frequently fails to measure the blood pressure values, or the values measured are too low (too high).	1. Check the positioning of the cuff. 2. Measure the blood-pressure again in peace and quiet under observance of the details made under point 5.
Every measurement produces a different value although the instrument functions normally and the values displayed are normal	1. Please read the following information and the points listed under «Common sources of error». Repeat the measurement. Please note: Blood pressure fluctuates continually so successive measurements will show some variability.
Blood pressure measured differs from those values measured by the doctor.	1. Record the daily development of the values and consult your doctor. Please note: Individuals visiting their doctor frequently experience anxiety which can result in a higher reading at the doctor than obtained at home under resting conditions.

10. CARE AND MAINTENANCE, RECALIBRATION

- Do not expose the device to either extreme temperatures, humidity, dust or direct sunlight.
- The cuff contains a sensitive air-tight bubble. Handle this carefully and avoid all types of straining through twisting or buckling.
- Clean the device with a soft, dry cloth. Do not use petrol, thinners or similar solvent. Spots on the cuff can be removed carefully with damp cloth and soapsuds. The cuff must not be washed!
- Do not drop the instrument or treat it roughly in any way. Avoid strong vibrations.
- Never open the device! Otherwise the manufacturer calibration becomes invalid!

11. BATTERY LIFE


1000 times measurement with 4- size "AAA" alkaline Batteries

12. BATTERY LIFE

⚠ Safety and protection

- This instrument maybe used only for the purpose described in this booklet. The manufacturer cannot be held liable for the damage caused by incorrect application.
- This instrument comprises sensitive components and must be treated with caution. Observe the storage and operating condition described in the "Technical specifications" section!



- Protect it from water and moisture, extreme temperatures, impact and dropping, contamination and dust, direct sunlight, heat and cold
- The cuffs are sensitive and must be handled with care
- Only pump up the cuff once fitted
- Do not use the instrument close to strong electromagnetic fields such as mobile telephones or radio installations
- Do not use the instrument if you think it is damaged or notice anything unusual.
- If the instrument is not going to be used for a prolonged period the batteries should be removed.
-  Read the additional safety instructions in the individual sections of this booklet. Ensure that children do not use the instrument unsupervised: some parts are small enough to be swallowed
- Must use the recognized accessories, detachable parts and materials, if the use of other parts or materials can degrade minimum safety
- A warning to remove primary batteries if the instruments is not likely to be used for some time

Instrument care

Clean the instrument only with a soft, dry cloth

Disposal







Batteries and electronic instruments must be disposed of in accordance with the locally applicable regulations, not with domestic's waste.

13. REFERENCE TO STANDARDS







Device standard: Device corresponds to the requirements of the European standard for non-invasive blood-pressure monitor

Standard
IEC60601-1-6:2010+A1:2013/ EN60601-1-6:2010+A1:2015
IEC60601-1:2005+A1:2012/EN60601 1:2006+A11:2011+A1:2013+A12:2014
IEC60601-1-2:2014/ EN60601-1-2:2015
IEC/EN60601-1-11:2015
IEC80601-2-30:2009+A1:2013/EN80601-2-30:2010+A1:2015

14. REMARK

	Some electrical and electrical equipment forbid to abandon and disposal at will	 0197	Some electrical and electrical equipment forbid to abandon and disposal at will
	Manufacturer's name and address		Reading Instruction Book before use



	Inapplicable baby		Type BF equipment
	Cuff Connector		Keep Dry
	Attention consult accompanying documents		MedNet EC-REP GmbH, Borkstrasse 10, 48163 Münster, Germany

15. TECHNICAL SPECIFICATIONS

Measurement Procedure:	Oscillometric, corresponding to Korotkoff method: Phase I: systolic, Phase V: diastolic
Display:	Digital display
Measuring range:	SYS/DIA: 30 to 280 mmHg (in 1 mmHg increment) Pulse: 40 to 199 beat/minute
Static accuracy:	SYS/DIA: ± 3 mmHg / Pulse: $\pm 5\%$ of reading

Measuring resolution:	1mmHg
Inflation:	Automatic inflation by internal pump
Memory function:	SYS/DIA: 30 to 280 mmHg (in 1 mmHg increment) Pulse: 40 to 199 beat/minute
Static accuracy:	2 x 120 memories for 2 users (SYS, DIA, Pulse)
Decompression:	Constant exhaust valve system
Power source:	4-size "AAA" alkaline batteries
Operation temperature:	5-40°C/41-104°F
Operation humidity:	15%-80%RH maximum
Storage temperature:	-20-+55°C/-4-+131°F
Storage humidity:	10%-95%RH maximum
Dimensions:	148 x 94 x 60 ± 1.0 mm
Weight:	373 g ± 5 g (including batteries and cuff)
Cuff pressure display range:	0-290mmHg/0-38.7KPa
Electrical shock protection:	Internal power unit
Safety classifications:	Type BF equipment
Mode of operation:	Continuous operation



Protection against ingress of water:	Ip22
Accessories:	M-L Size Cuff, 4 "AAA" batteries, instruction manual

● 16. MANUFACTURER'S DECLARATION ●

The Dr Trust BP Check Pro - 123 is intended for use in the electromagnetic environment specified below. The customer or the user of the Dr Trust BP Check Pro - 123 should assure that it is used in such an environment.

Electromagnetic Emissions: (IEC60601-1-2)

Emission Test	Compliance	Electromagnetic Environment
RF emission CISPR 11	Group 1	The Dr Trust BP Check Pro-123 uses RF energy only for internal functions. Therefore, this RF emission is extremely weak and there is little chance of it creating any kind of interference whatsoever with nearby electronic equipment.

Emission Test	Compliance	Electromagnetic Environment
RF emissions CISPR 11	Class B	The Dr Trust BP Check Pro-123 is suitable for use in all establishments, including domestic establishments and those directly connected to the public low voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Not applicable	
Voltage fluctuations/flicker IEC 61000-3-3	Not applicable	

Electromagnetic Immunity: (IEC60601-1-2)


Immunity test	IEC60601-1-2 test level	Compliance level	Electromagnetic environment -guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30 %.
Electric fast transient/burst IEC 61000-4-4	±2 kV for power supply lines ±1 kV for input/output lines	Not applicable	Mains power quality should be that of a typical commercial or hospital environment.



Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	Not applicable	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5 % UT 95% dip in UT for 0.5 cycle 40 % UT 60% dip in UT for 5 cycles 70 % UT (30% dip in UT) for 25 cycles <5 % UT 95% dip in UT for 5 sec.	Not applicable	Mains power quality should be that of a typical commercial or hospital environment. If the user of the upper arm style requires continued operation during power mains interruptions, it is recommended that the Dr Trust BP Check Pro-123 be powered from an uninterruptible power supply or a battery.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m	Not applicable	Not applicable
Note: UT is the a.c. mains voltage prior to application of the test level.			

Immunity test	IEC60601-1-2 test level	IEC60601-1-2 test level	Electromagnetic environment -guidance
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz 80% AM (2Hz)	3 Vrms	Portable and mobile RF communications equipment should be used no closer to any part of the Dr Trust BP Check Pro-123, including cables, than their commended separation distance calculated from the equation applicable to the frequency of the transmitter. Recommend separation distance 3V $d = 1.2 \times p^{1/2}$ 80MHz to 800 MHz $d = 2.3 \times p^{1/2}$ MHz to 2.5 GHz where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer



Radiated RF IEC 61000-4-3	3 Vrms 80 MHz to 2.5 GHz 80% AM (2Hz)	3 V/m	and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range. Interference may occur in the vicinity of equipment marked with the following symbol: 
---------------------------	---------------------------------------	-------	--

Note1: At 80 MHz and 800 MHz, the higher frequency range applies.

Note2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects, and people.

<p>a Field strength from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the Dr Trust BP Check Pro-123 is used exceeds the applicable RF compliance level above, the Dr Trust BP Check Pro-123 should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the BPCB0A-2H.</p> <p>b Over the frequency range 150 kHz to 80MHz, field strengths should be less than 3 V/m.</p> <p>Recommended Separation Distances: Recommended separation distance between portable and mobile RF communications equipment and the Dr Trust BP Check Pro-123 The Dr Trust BP Check Pro-123 is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the Dr Trust BP Check Pro-123 can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the Dr Trust BP Check Pro-123 as recommended below, according to the maximum output power of the communications equipment.</p>			
Rated maximum output power of transmitter (W)	Separation distance according to frequency of transmitter m		
	150 kHz to 80 MHz $d = 1.2 \times p^{1/2}$	80 MHz to 800 MHz $d = 1.2 \times p^{1/2}$	800 MHz to 2.5 GHz $d = 2.3 \times p^{1/2}$



0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be determined using the equation applicable to the frequency of the transmitter, where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note1: At 80MHz and 800MHz, the separation distance for the higher frequency range applies.

Note2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

15. CUSTOMER SUPPORT

CONTACT ADDRESS

USA

Nureca INC.USA
276 5th Avenue, Suite 704-397,
New York (NY) - 10001, USA

INDIA

Corporate Office (Mumbai)

Nureca Limited
128 Gala Number Udyog Bhavan,
1st Floor Sonawala Lane, Goregaon East
Mumbai City Maharashtra 400063

Contact us

India: +91-7527013265 / +91-9356658436

Website: www.drtrust.in

Corp Website: www.nureca.com

Email: customercare@nureca.com

Connect with us on social networks

Facebook: @drtrust

Instagram: @drtrustisin

Youtube: NurecaUsa



Scan to View
Product Demo Video
www.drtrustusa.com/123

COPYRIGHT ©2021 NURECA LTD ALL RIGHTS RESERVED